

B-Bridge International, Inc.



Human Resistin ELISA Kit User Manual

UM-100301
Published 01 August 2004
Catalog# K1003-1

See List of Components for Storage Conditions
FOR RESEARCH USE ONLY

Table of Contents

I.	Introduction and Protocol Overview	3
II.	List of Components	5
III.	Additional Materials Required	6
IV.	Reagent Preparation and Storage	7
V.	Sample Preparation	8
VI.	Human Resistin ELISA Protocol	9
VII.	Calculation of Results	11
VIII.	Troubleshooting Guide	12
IX.	References	13

Notice to Purchaser

This product is to be used for Research Purposes Only. It is not to be used for Drug or Diagnostic Purposes, nor is it intended for Human Use. B-Bridge products may not be resold, modified for resale, or used to manufacture commercial products without the express written consent of B-Bridge International, Inc.

EXCEPT AS OTHERWISE EXPRESSLY SET FORTH IN THIS USER MANUAL, B-BRIDGE DOES NOT MAKE ANY REPRESENTATION OR WARRANTIES OR CONDITIONS OF ANY KIND, EITHER EXPRESSED OR IMPLIED, WITH RESPECT TO THE PRODUCTS, OR INFORMATION DISCLOSED HEREUNDER, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY, FIT FOR A PARTICULAR PURPOSE, OR NONINFRINGEMENT OF THE INTELLECTUAL PROPERTY RIGHTS OF THIRD PARTIES.

©2004, B-Bridge International, Inc. All Rights Reserved.

I. Introduction and Protocol Overview


Resistin, a product of the RSTN gene, is a peptide hormone belonging to the class of cysteine-rich secreted proteins which are termed the RELM family, and is also described as ADSF (Adipose Tissue-Specific Secretory Factor) and FIZZ3 (Found in Inflammatory Zone). Human resistin contains 108 amino acids as a pre-peptide. Its hydrophobic signal peptide is cleaved before it is secreted. Resistin circulates in human blood as a dimeric protein consisting of two 92 amino acid polypeptides, which are disulfide-linked via Cys26.

Resistin may be an important link between obesity and insulin resistance. Mouse resistin, specifically produced and secreted by adipocytes, acts on skeletal muscle myocytes, hepatocytes and adipocytes themselves to reduce their sensitivity to insulin. Stepan et al. (2001) have suggested that resistin suppresses the ability of insulin to stimulate glucose uptake. They have also suggested that resistin is present at elevated levels in blood of obese mice, and is down regulated by fasting and antidiabetic drugs. Way et al. (2001), on the other hand, have found that resistin expression is severely suppressed in obesity and is stimulated by several antidiabetic drugs. Other studies have shown that mouse resistin increases during the differentiation of adipocytes, but it also seems to inhibit adipogenesis. In contrast, the human adipogenic differentiation is likely to be associated with a down regulation of resistin gene expression.

The B-Bridge **Human Resistin ELISA Kit** is designed to measure the concentration of human resistin in human serum, plasma, or tissue culture medium.

The principle of the assay is shown in Figure 1. Standards or samples are incubated in microtiter wells coated with a goat polyclonal anti-human resistin antibody. The wells are washed, and a biotin-labeled rabbit polyclonal anti-human resistin antibody is added and incubated with the captured resistin. After a thorough wash, streptavidin-horseradish peroxidase conjugate is added. Following subsequent incubation and washing, the bound conjugate is allowed to react with the substrate H_2O_2 -tetramethylbenzidine (TMB). The reaction is quenched by addition of acidic solution and absorbance of the resulting product is measured at 450 nm. The absorbance is proportional to the concentration of resistin. A standard curve is constructed by plotting absorbance values versus resistin concentrations of calibrators, and concentrations of unknown samples are determined using this standard curve.

Figure 1. Assay Principle

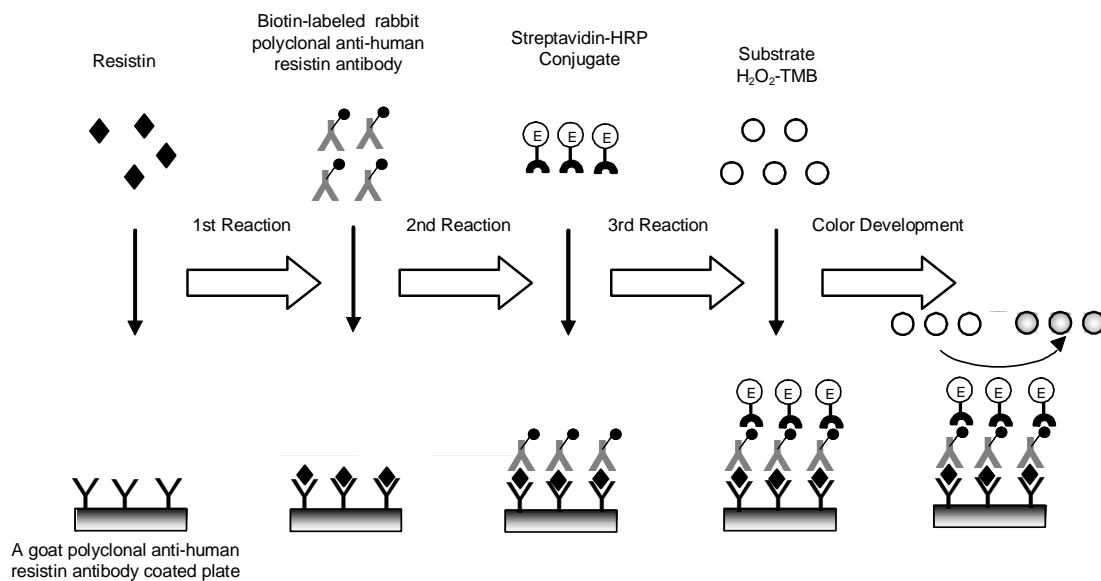

II. List of Components

- **Store all components at 2-8°C. DO NOT FREEZE.**

1	10X WASH SOLUTION	1 Bottle (100 ml)
2	1X SAMPLE DILUENT	2 Bottle (10 ml each)
3	PRIMARY ANTIBODY-COATED PLATE One plate holds 12x8-well strips (96 wells), with adsorbed Goat Polyclonal Anti-Human Resistin Antibody. Plate is provided in a resealable foil pouch with desiccant.	1 Plate
4	HUMAN RESISTIN MASTER STANDARD Lyophilized	1 Vial (50ng)
5	QUALITY CONTROL High and Low, lyophilized	2 Vials
6	BIOTINYLATED SECONDARY ANTIBODY SOLUTION Rabbit Polyclonal Anti-Human Resistin Antibody, Biotin Labeled	1 Bottle (13 ml)
7	CONJUGATE SOLUTION Streptavidin-Horseradish Peroxidase Conjugate	1 Bottle (13 ml)
8	SUBSTRATE H ₂ O ₂ Tetramethylbenzidine	1 Bottle (13 ml)
9	STOP SOLUTION (0.2M H ₂ SO ₄)	1 Bottle (13 ml)

MSDS forms are available on our website—please visit www.b-bridge.com

III. Additional Materials Required

The following materials are required, but not supplied:

- Graduated cylinder
- Micropipettor(s) and disposable pipette tips
- Null strips for 96-well plate
- 96-well plate washer
- Paper towels or absorbent paper
- Plate reader capable of measuring absorbance at a wavelength of 450 nm
- Orbital microplate shaker capable of approximately 300 rpm
- Tubes for sample dilutions
- Deionized water

IV. Reagent Preparation and Storage

Allow all the reagents to equilibrate at room temperature (25°C) prior to the start of the reagent preparation.

1. 1X Wash Solution

Prepare 1X Wash Solution by mixing 100 ml of 10X Wash Solution with 900 ml of deionized water or equivalent. After preparation, store 1X Wash Solution at 2-8°C. The diluted Wash Solution is stable for 1 month at 2-8°C.

2. Human Resistin Standard Solution

Reconstitute the Resistin Master Standard with 1 ml of 1X Sample Diluent. Prepare each Resistin Standard (20 ng/ml, 10 ng/ml, 5 ng/ml, 2 ng/ml, and 1 ng/ml) by serially diluting the stock Resistin Master Standard Solution (50 ng/ml) with 1X Sample Diluent as shown in the table. Use the reconstituted Resistin Standard (50 ng/ml) and 1X Sample Diluent for the 50.0 ng/ml and 0 ng/ml standard solutions, respectively.

Table 1: Serial Dilution of Resistin Standards

Master Standard Vol.	1X Diluent	Concentration
Master Std. Stock	-	50 ng/ml
500 µl of Master Std. Stock	750 µl	20 ng/ml
500 µl of 20 ng/ml Std.	500 µl	10 ng/ml
500 µl of 10 ng/ml Std.	500 µl	5 ng/ml
500 µl of 5 ng/ml Std.	750 µl	2 ng/ml
500 µl of 2 ng/ml Std.	500 µl	1 ng/ml

Further dilute the serial diluted Standard Solutions 1:3 prior to use by mixing 100 µl of Standard Solutions with 200 µl of Sample Diluent for duplicates. Do not store the diluted standard solutions.

Reconstituted and undiluted Resistin Standard Solutions should be frozen at -20°C for the next use. Do not store the diluted (1:3) standard solutions.

3. Quality Controls

Reconstitute the Quality Controls with 350 µl Sample Diluent, mix and let sit for 30 minutes at room temperature. Further dilute the reconstituted Quality Controls 1:3 with Sample Diluent prior to use (50 µl control + 100 µl Sample Diluent for singlets or 100 µl Quality Control + 200 µl Sample Diluent for duplicates). Reconstituted Quality Controls are stable until the expiration date at 2-8°C. Do not store the 1:3 diluted Quality Controls.

V. Sample Preparation

Allow all the reagents to equilibrate at room temperature (25°C) prior to the start of the sample preparation.

1. For Assaying Samples in singlets
Mix 50 µl of samples with 100 µl of Sample Diluent.
2. For Assaying Samples in duplicates
Mix 100 µl of samples with 200 µl of Sample Diluent.

Do not store 1:3 diluted samples.

VI. Human Resistin ELISA Protocol

Note: Allow all reagents to equilibrate at room temperature (25°C) prior to the start of the assay and prepare 1X Wash Solution, Quality Controls, Resistin Standards, and samples as described in the previous sections.

1. Remove Primary Antibody-Coated Plate from its foil pouch. Remove any unneeded strips from the plate frame, reseal them in the foil pouch, and return the foil pouch to 2-8°C. If a 96-well plate washer is used, the plate frame should be completely filled with wells by adding as many null strips as necessary. Identify well position(s) for each sample on a data sheet or plate map.
2. Add 100 µl of diluted Standards, Quality Controls, Sample Diluent (blank) and samples to the appropriate number of antibody-coated wells. Every plate must include the standard series to properly correlate the sample readings.
3. Cover plate(s) securely and incubate at room temperature (25°C) for 60 minutes on an orbital microplate shaker at ca. 300 rpm.
4. After incubation, wash the plate(s) 3 times with Wash Solution as follows:
 - a. Completely aspirate the liquid from the wells using a plate washer.
 - b. Fill each well with 1X Wash Solution (~350 µl/well) and immediately aspirate. Avoid overflow.
 - c. Repeat Step 4b two more times for a total of three washes.
 - d. Invert the plate(s) and gently tap on a clean absorbent towel.
5. Dispense 100 µl of the Biotinylated Secondary Antibody Solution into each well.
6. Cover plate(s) securely and incubate at room temperature (25°C) for 60 minutes on an orbital microplate shaker at ca. 300 rpm.
7. Repeat the wash procedure described in step 4.
8. Dispense 100 µl of Conjugate Solution into each well.
9. Cover plate(s) securely and incubate at room temperature (25°C) for 60 minutes on an orbital microplate shaker at ca. 300 rpm.
10. Repeat the wash procedure described in step 4.
11. Dispense 100 µl of Substrate Solution into each well. Avoid exposing the microtiter plate to direct sunlight. Covering the plate with aluminum foil is recommended.
12. Cover plate(s) securely and incubate at room temperature (25°C) for 10 minutes with no shaking. The incubation time may be extended up to 20 minutes, if the reaction temperature is below 20°C.
13. Dispense 100 µl of Stop Solution into each well. The plate should be read immediately.
14. Read the plate at 450 nm using a plate reader.

Note: If the microplate reader is not capable of reading absorbance greater than the absorbance of the highest standard, the standard curve constructed using the values measured at 405 nm can be used to determine leptin concentration of off-scale samples. The readings at 405 nm should not replace the on-scale readings at 450 nm.


Figure 2. Flow Chart of Assay Procedure



VII. Calculation of Results

1. Subtract the mean absorbance value of the 0 ng/ml blank from each mean absorbance value of the standard series and samples tested (Net Absorbance).
2. Plot the log of known concentrations of each standard and the calculated Net Absorbances on the X-axis and Y-axis, respectively. Fit an appropriate regression curve to the plotted points.
3. Determine the resistin concentrations of the samples by interpolation of the regression curve formula.

Figure 3. Typical Standard Curve

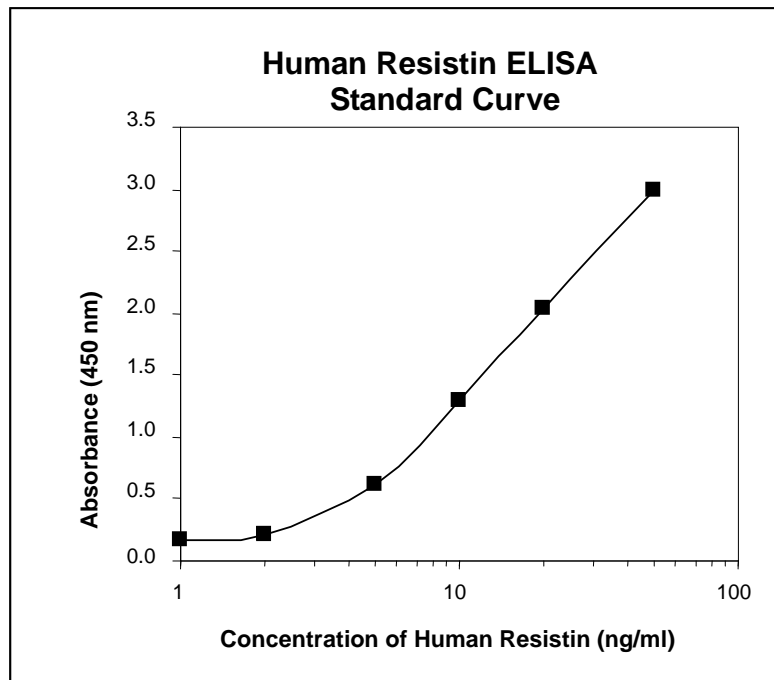

VIII. Troubleshooting Guide

1. Lack of signal or weak signal in all wells

Possible explanations:

- Omission of a reagent or a step.
- Improper preparation or storage of a reagent.
- Assay performed before reagents were allowed to come to 25°C.
- Plate reader did not perform well.

2. High signal and background in all wells

Possible explanations:

- Improper or inadequate washing; be certain that all wash volumes and repetitions were correct.
- Decrease color development time.
- The plate should be read within 5 minutes of stopping the color development

3. High background in sample wells only

Possible explanations:

- Sample concentration was too high.

4. Weak signal in sample wells only

Possible explanations:

- Sample concentration was too low.

IX. References

- Banerjee R.R., Lazar M.A.: Dimerization of resistin and resistin-like molecules is determined by a single cysteine. *The Journal of Biological Chemistry*. 276, 25970-25973, (2001)
- Fasshauer M. et al.: Tumor Necrosis Factor α Is a Negative Regulator of Resistin Gene Expression and Secretion in 3T3-L1 Adipocytes. *Biochemical and Biophysical Research Communications*. 208, 1027-1031, (2001)
- Hartman H.B., Lazar M.A. et al.: Mechanisms Regulating Adipocyte Expression of Resistin. *The Journal of Biological Chemistry*. 277 (22), 19754-19761, (2002)
- Juan CC. et al.: Suppressed Gene Expression of Adipocyte Resistin in an Insulin-resistant Rat Model Probably by Elevated Free Fatty Acids. *Biochemical and Biophysical Research Communications*. 289, 1328-1333, (2001)
- Kim KH. et al.: A Cysteine-rich Adipose Tissue-specific Secretory Factors Inhibits Adipocyte Differentiation. *The Journal of Biological Chemistry*. 276 (14), 11252-11256, (2001)
- Steppan C.M., Lazar M.A.: Resistin and obesity-associated insulin resistance. *TRENDS in Endocrinology and Metabolism*. 13 (1), 18-23, (2002)
- Steppan C.M. et al.: The Hormone Links Obesity to Diabetes. *Nature*. 409, 307-312, (2001)
- Steppan C.M. et al.: A Family of Tissue-specific Resistin-like Molecules. *Proc. Natl. Acad. Sci. USA*. 98 (2), 502-506, (2001)
- Way J.M. et al.: Adipose Tissue Resistin Expression Is Severely Suppressed in Obesity and Stimulated by Peroxisome Proliferator-activated Receptor γ Agonists. *The Journal of Biological Chemistry*. 276 (28), 25651-25653, (2001)